

PHILOSOPHY HF 400



High frequency x-ray unit – touch screen – automatic

Philosophy HF 400

X-ray unit designed for
CR – DR digital systems

 IPS Medical

Philosophy HF 400



**Head rotation
+/- 90° (optional)**



**Removable
x-ray grid**



**X-ray steel
plate cassette**



**Cleat rope ties
(optional)**

COLLIMATOR

- Patient support table 4 ways with mechanical brakes**
- Max weight capacity for patient support table 100 Kg**
- Table absorption thickness 5 mm 0,8 mm**
- Film focus distance 100 cm**
- Multilayer**
- Variable field from 0x0 to 43x43 cm, 100 cm DDF**
- High intensity halogen lamp 160 lux at 100 cm**
- Lamp timer at 30s**

Philosophy HF 400

Selectable operating system



technique

3 points

2 points



Automatic anatomic programme



- PC touch screen 15" multi-language run by processor
- 100 programmed anatomical parts, reprogrammable by the operator
- 19 different patient weights
- 4 reinforcement pattern speed
- USB port for software updates

Philosophy HF 400

X-ray Generator

- Monoblock
- Max Power 30 kW
(300 mA - 100 kV - 100 mS)
- Max Voltage 99 kV - 125 kV
- Max Power Supply 400 mA
- Frequency ripple 40 KHZ
- Ripple 1%
- Monoblock heat capacity 825 kJ - 1103 KHU

X-ray Tube


- X-ray tube with rotating anode 3000 rpm
- Focal spot 0,6-1,3 mm
- Anode angle 15°
- Heat capacity 80kJ - 107 KHU
- Continuous thermal dissipation max anode 300 W

Power Supply

- Standard Voltage 230/240 V ± 10% 50-60 Hz
- Line resistancy 0,4 Ω
- Power consumption < 1A

Safety and protection

- Filament current safety and automatic control
- Overcurrent and overvoltage protection (kV e mA)
- X-ray tube load protection
- Reporting errors or malfunction

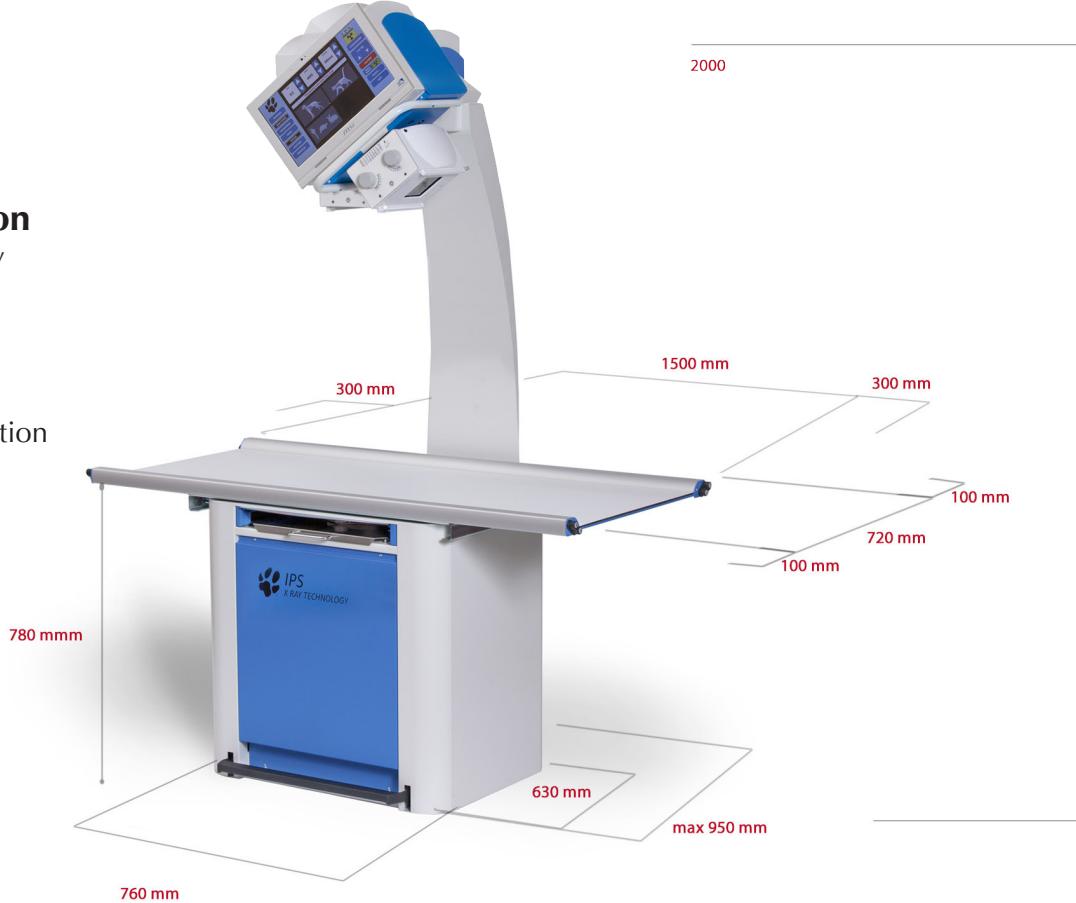

- Selection of mA in 7 values from 80 to 400 mA
- Selection of exposure time from 0,003 to 2 sec.
- Continuous selection of kV from 40 to 125 kV
- Selection of 25 max values 125 - 250 mAs (optional)



I.P.S. MEDICAL SRL

Via Vassanelli 16/D – 37012 BUSSOLENGO (VR) - Italy
Tel. 045-6702927 Fax 045-6702927 ips@ipsxray.com

www.ipsxray.com